CHARMGIRL

User’s Manual F-100

4 in 1 V10 big handle

(RF + 40k cavitation +Vacuum + Infrared ray light + BIO)
Cryolipolysis +Cooling plates Slimming machine

GUANGZHOU MEIZI BEAUTY EQUIPMENT FACTORY

NOTES

1 Please take and put the handle gently and do not fall it on the floor.
2 In case of first use of cryoprobe, The machine water tank must be filled with water. (when the water outflow from overflow outlet. It means the machine is already filled of water.)
3 Add water to the machine on a regular basis (often supplement once a week). The water in the water tank must be discharged during packaging and transporting of the equipment.
4 The equipment shall stop for 10 minutes after one hour ' s work. Continuous high - intensity use will shorten the service life of the equipment.
5 Do not use the viscous media such as gel, which will block the tra - cheal.
6 You can use the alcohol to clean the handles, please avoid the alcohol to drop into the vacuum pipe, or touch the plastic which is protect the lights on this handle.

NOTES AFTER OPERATION

1) Avoid using cold water to clean the operation area within eight hours after operation(except facial part)；

2) Prohibit to do massage in the operation parts ；

3) Can’t smear moisturizing skin care products in the treatment parts；

FORBIDDEN GROUP

1). People with heart disease or high blood pressure, or configured cardiac pacemaker.

2). Patients with acute inflammation, asthma, deep vein thrombosis, cancer, etc.

3). People with hemorrhagic disease, trauma or who is bleeding.

4). Pregnant women

5). Medical Plastic parts, or parts with artificial in filling inside.

6). People with metal inside the body(include metallic tooth)

7). Patient with skin inflammation or with edema.

8). People with an abnormal immune system.

9). Numb or insensitive to heat.

CATALOG

01 4 IN 1 V10 BIG HANDLE

02 FUNCTION INTRODUCTION

04 40KHZ ULTRASONIC CAVITATION FOR FAT EXPLODING

12 OPERATIONS

19 TECHNICAL PARAMETERS

THE INSTALLATION PROCESS

19

01

4 IN 1 V10 BIG HANDLE

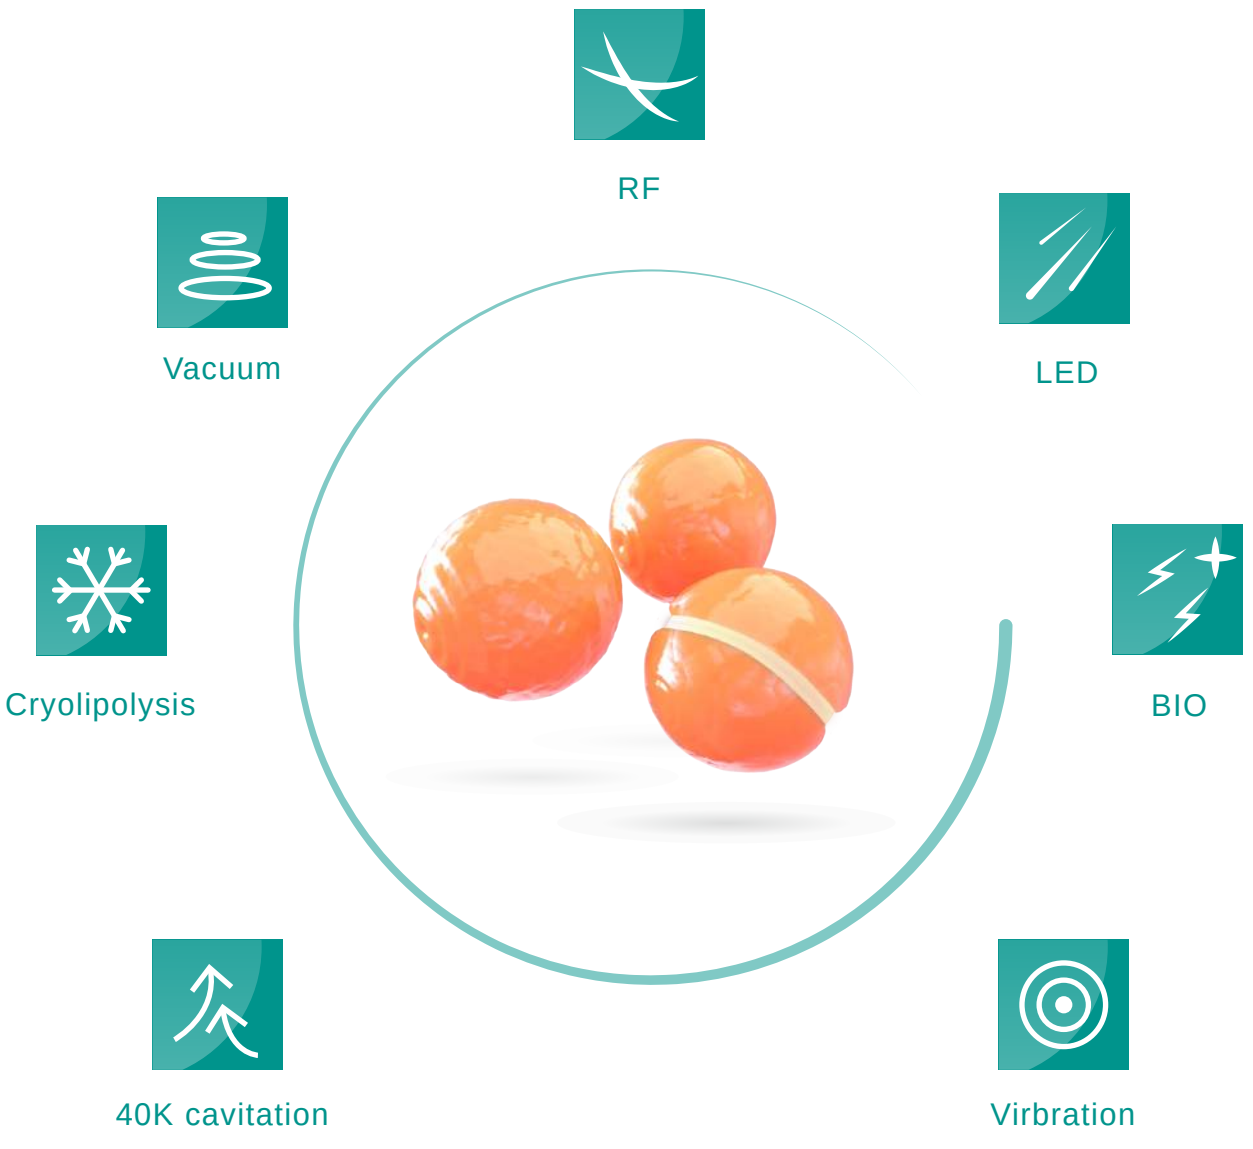

02 FUNCTION INTRODUCTION

✚ New 40khz cavitation handle

✚ Cryo therapy handle

✚ Cooling Plates
with Vibraion handle*4

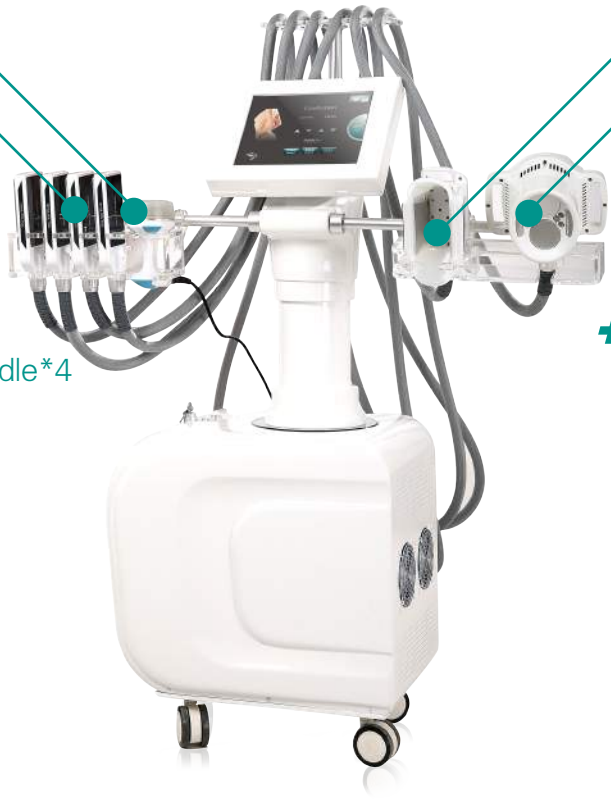

✚ V10 handle

Power:1000W
Voltage: 220V–240V/Hz 110V–130V/Hz
Packing size :120*76*68CM
Touch screen : 12.4 inches

1	The sheif
2	10.4"TFT COLOR touch screen
3	Ket switch
4	Cooling Plates with Vibration handle Socket 1
5	V10 handie Socket
6	Cooling Plates with Vibration handle Socket 2
7	Cooling Plates with Vibration handle Socket 3
8	Cryo therapy handle Socket
9	Cooling Plates with Vibration handle Socket 4
10	40khz cavitation handle Socket
11	inflow hole
12	Outfow hole
13	Power Plug

04

V10 handle[RF+40K cavitation +vacuum+IR+BIO all in one handle

Function

BIO:Purifying, detoxifying, promoting metabolism and fat burning, and to achieve better and faster shaping effective-ness

Cavitatio:Destroy and burn the fat cells, remove fat

LED:Enhance cellular activity, promote blood circulation and metabolism

Vacuum:Use negative pressure aspirator suction to excess subcutaneous fat

BIO

40k cavitation

LED

Vacuum

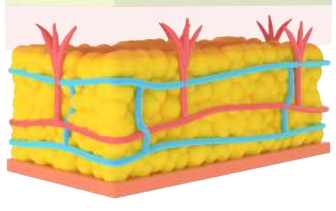

A

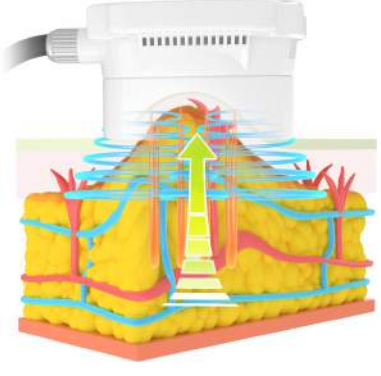

B

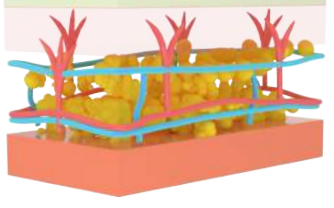

C

Before	Treatment	After
The 5 treatment for 10 days	The 5 treatment for 10 days	The 5 treatment for 10 days

05

Far infrared heating: it can get results of promoting blood circulation, increasing active oxygen and accelerating the detoxification.

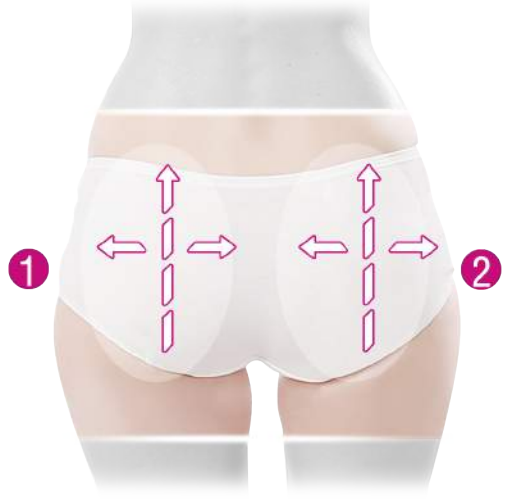

[20-15mins]

[20-15mins]

Function

Virbration:Promote the blood circulation, shaking fat

Cryolipolysis:Freeze and kill fat cells to eliminate from body

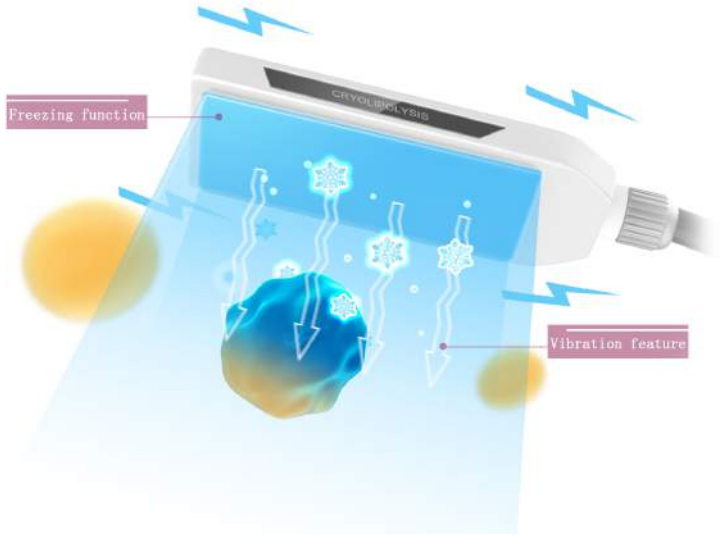

Virbration

Cryolipolysis

A B C

Before

The 5 treatment for 10 days

Treatment

The 5 treatment for 10 days

After

The 5 treatment for 10 days

Advantage

1, Intelligent management
2, Intelligent flow monitoring
3. Intelligent temperature
4. Large TFT screen display

07



Far infrared heating: it can get results of promoting blood circulation, increasing active oxygen and accelerating the detoxification.

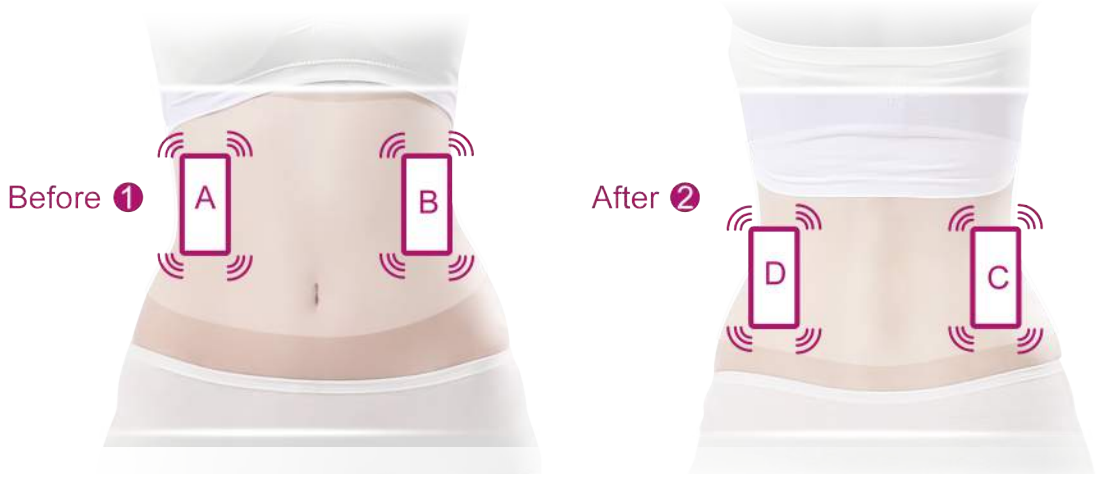

[20-15mins]

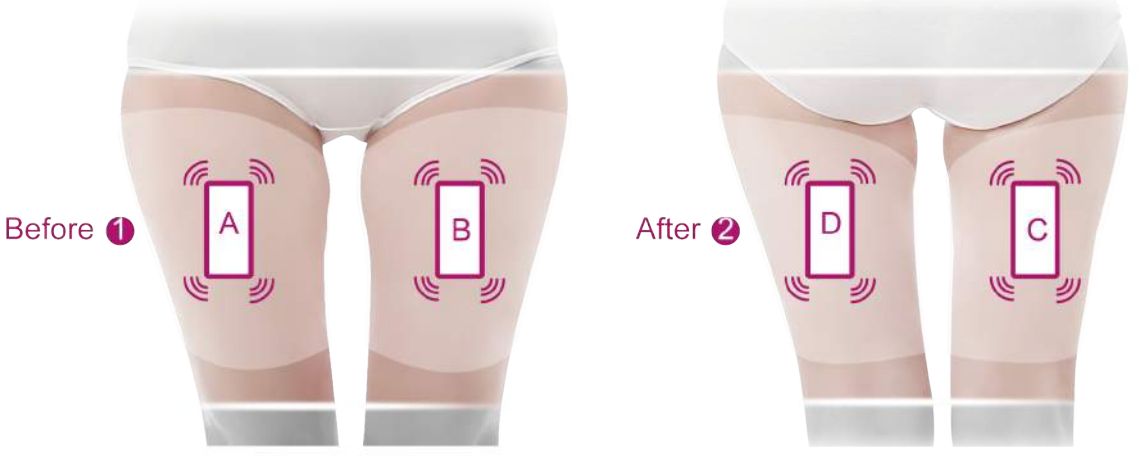

[20-15mins]

Function

Cavitatio:Destroy and burn the fat cells, remove fat

LED:Enhance cellular activity, promote blood circulation and metabolism

40k cavitation

LED

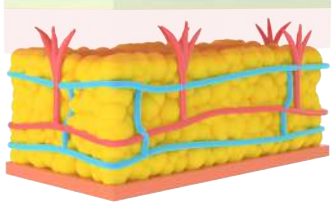

A

B

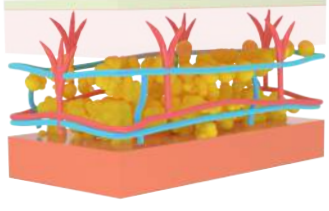

C

Before

The 5 treatment for 10 days

Treatment

The 5 treatment for 10 days

After

The 5 treatment for 10 days

Far infrared heating: it can get results of promoting blood circulation, increasing active oxygen and accelerating the detoxification.

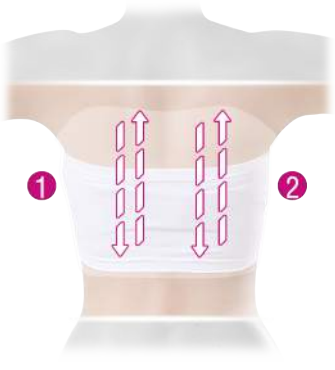

[20-15mins]

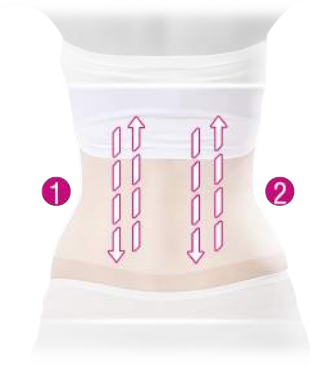

[20-15mins]

[20-15mins]

[20-15mins]

[20-15mins]

[20-15mins]

Function

Vacuum: Use negative pressure aspirator suction to excess subcutaneous fat

LED: Enhance cellular activity, promote blood circulation and metabolism

Cryolipolysis: Freeze and kill fat cells to eliminate

Vacuum

LED

Cryolipolysis

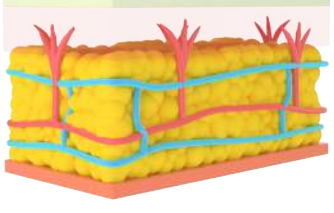

A

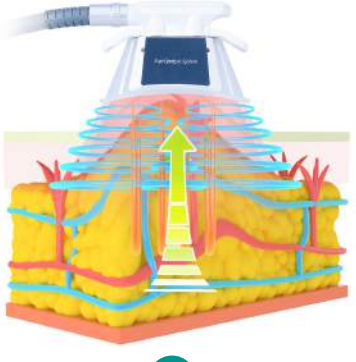

B

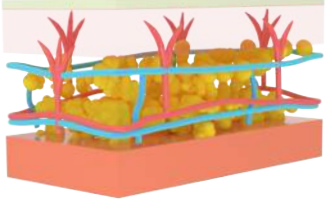

C

Before

The 5 treatment for 10 days

Treatment

The 5 treatment for 10 days

After

The 5 treatment for 10 days

Far infrared heating: it can get results of promoting blood circulation, increasing active oxygen and accelerating the detoxification.

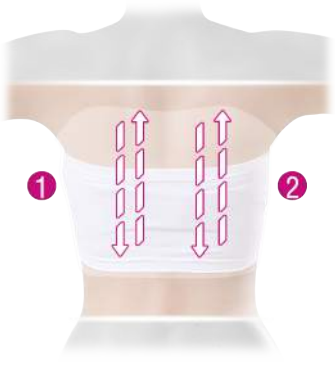

[20-15mins]

[20-15mins]

[20-15min]

[20-15mins]

[20-15mins]

[20-15mins]

Put on the power and turn on the key , it will enter into this interface, press “ENTER” in turn into the next operation interface,

1. Operating Instruction 1

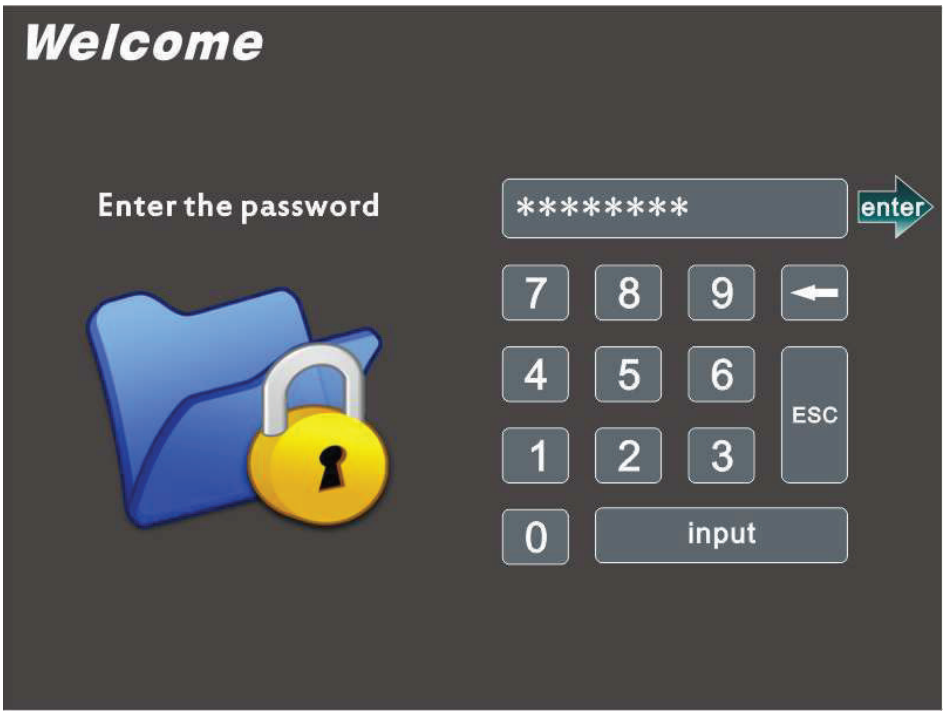

[Picture 1]

[Picture 2]

1.Cryolipolysis, V10 handle has own controlled screen
2.40K Cavitation handle and coolpads controlled by machine screen

2. Operating Instruction 2

1). V10 Magic Hi-Tech! RF+2x 40K cavi+vacuum+IR+BIO all in one handle

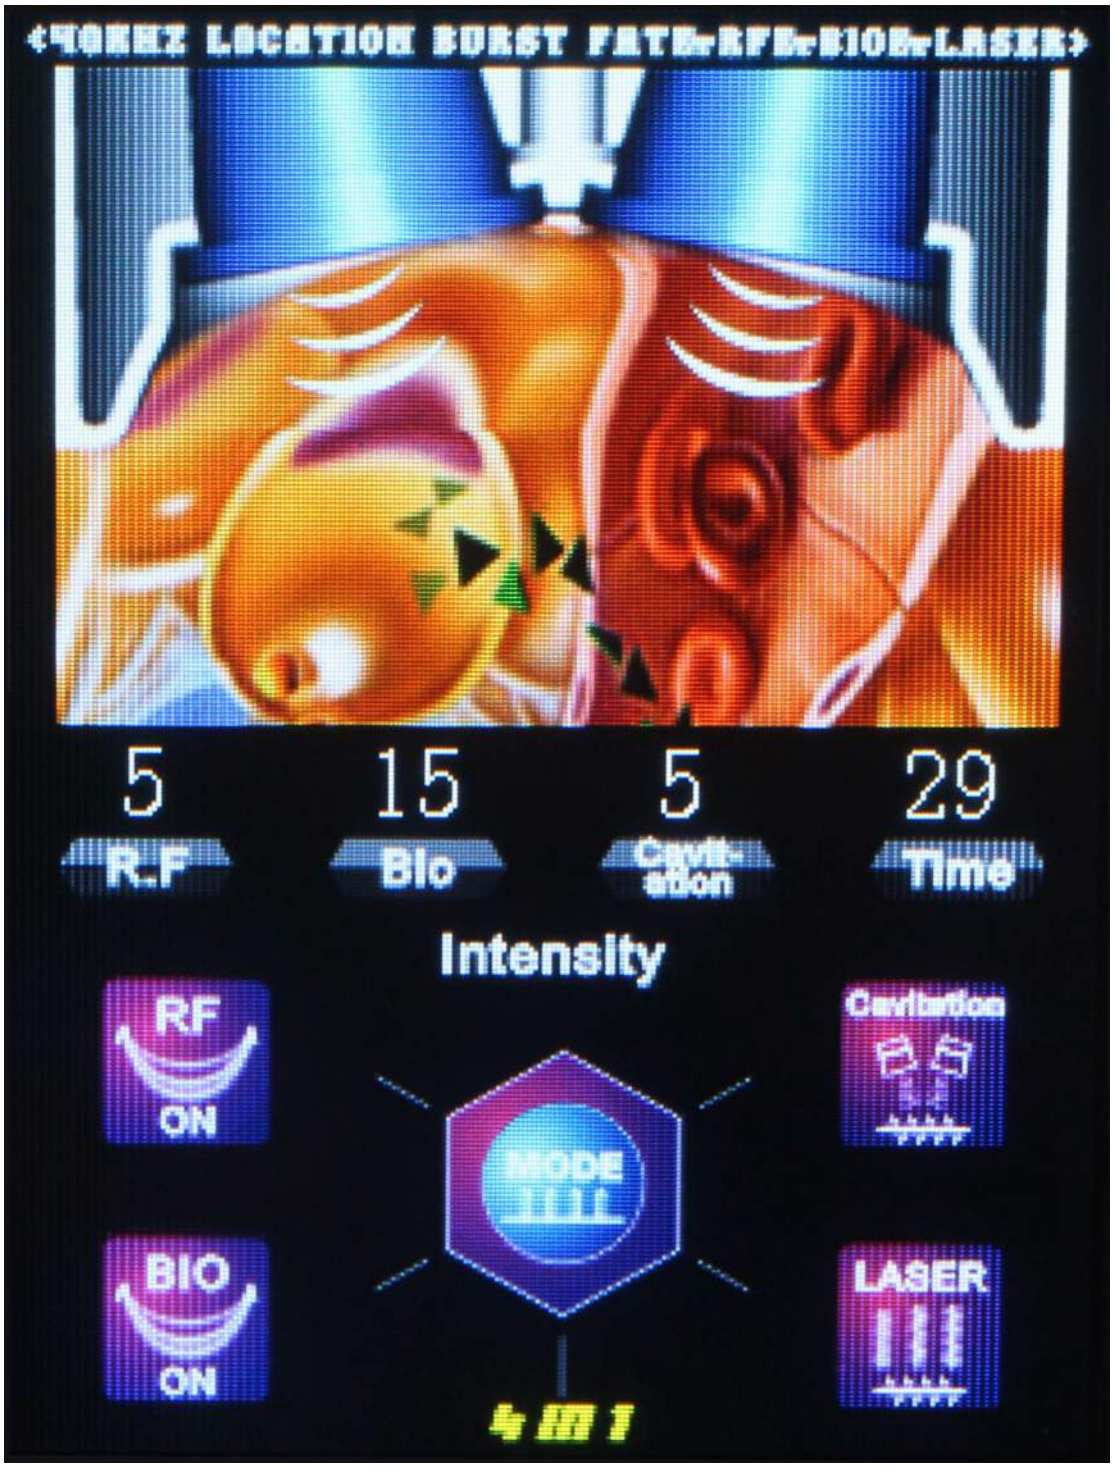

press “

” button to enter the operation interface of the big V10 handle, you can choose the Energy as you want, 1-10, suggest 4 or 5.

press “

” button to enter the operation interface of the big V10 handle, you can choose the Energy as you want, 1-15, suggest 6 or 7.

press “

” button to enter the operation interface of the big V10 handle, you can choose the Energy as you want, 1-10, suggest 6 or 7.

According to the customer's affordability, from low to high regulation as Energy.

2). Cryolipolysis handle

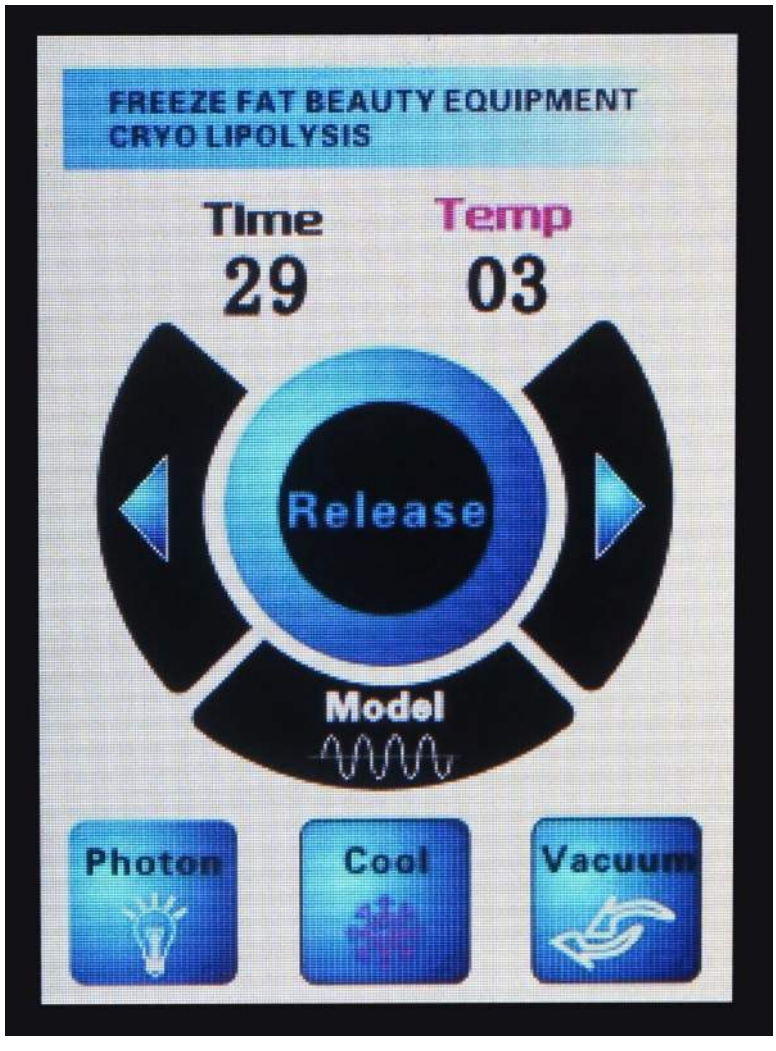

Handle Info

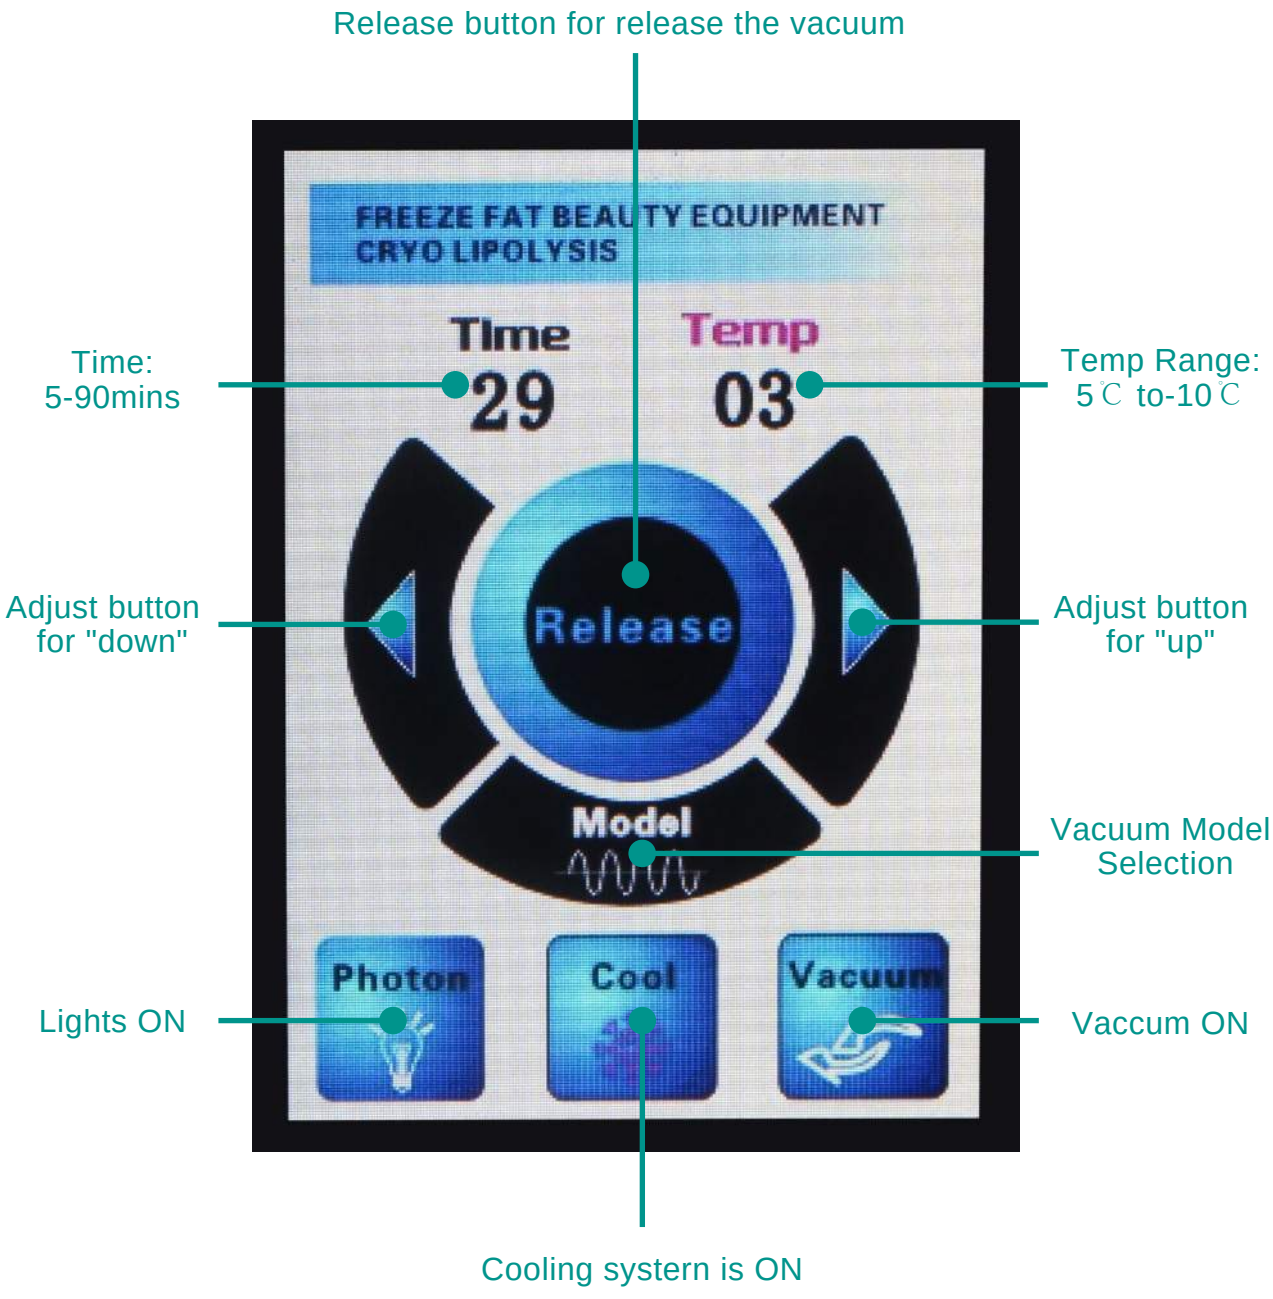
Release button for release the vacuum
FREEZE FAT BEAUTY EQUIPMENT
CRYO LIPOLYSIS
Time
Temp
Time:
5-90mins
29
03
Temp Range:
5℃ to-10℃
Release
Adjust button
for "down"
Adjust button
for "up"
Model
Vacuum Model
Selection
Photon
Cool
Vacuum
Lights ON
Vaccum ON
Cooling systern is ON

How to use the cryoprobe

A. First please put on the anti-freezing membrane on the skin before used the cryo-probe.

B. For the first treatment of the cryoprobe, please adjust the temperature to 5℃ or 3℃for 5 minutes and then adjust the temperature to 0℃for about 5 minutes ,and then -3℃ or-5℃ for 10~15 mins.

C. For the next treatment (Note: please don't treat the same parts more than one time in one month period).

Operation 1

1. Skin cleaning.
2. Apply the Anti-freezing membrane on the treatment area .
3. Apply the vacuum cryoprobe on the treatment parts

Operation 2

1). Please touch here

, when it turns to be red like this, then you can adjust arrows on both sides to change the temperature level . Please adjust the operation time like this above method.

2)

Touch to start or stop the infrared light. When it turns to red, it means it is working.

3)

Touch here to start the freezing.

4)

Touch here to start and stop the vacuum suction.

5)

Here can adjust the vacuum models. It has two models, one is long suction model and the other is suction and release every 0.5 seconds.

6)

Also you can touch here to release the vacuum.

3). 40K Cavitation handle

Strong sound wave explosion fat head

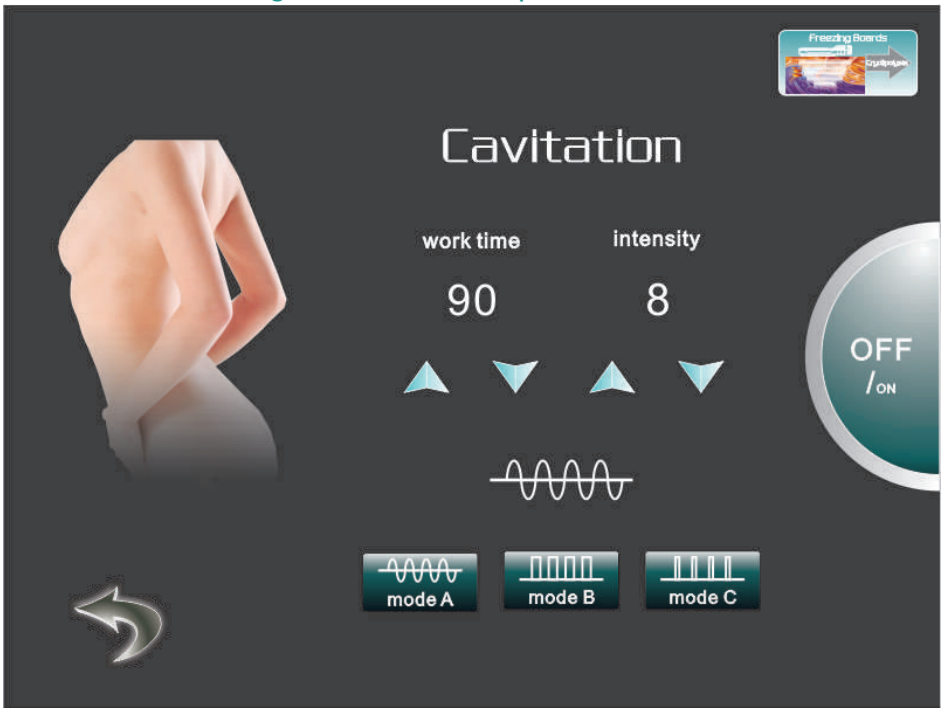

Press "work time" to adjust the time, press "▼" to decrease the strength or Press "▲" to increase the Energy. Press "OFF /ON" to start , act on the treatment area . Move in circularity, left to right side (right to left side), or downside to upside.

(Strong sound save explosion fat head may reach the fat layer directly by using strong sound, vibrate in-depth stubborn fat at top speed and produce numerous vacuum air pockets inside and outside the fat cells, robustly impact fat cells to generate introverted blast and disintegrate fat into free fatty acids.)

3). 4 pcs of Cooling plates with vibration system

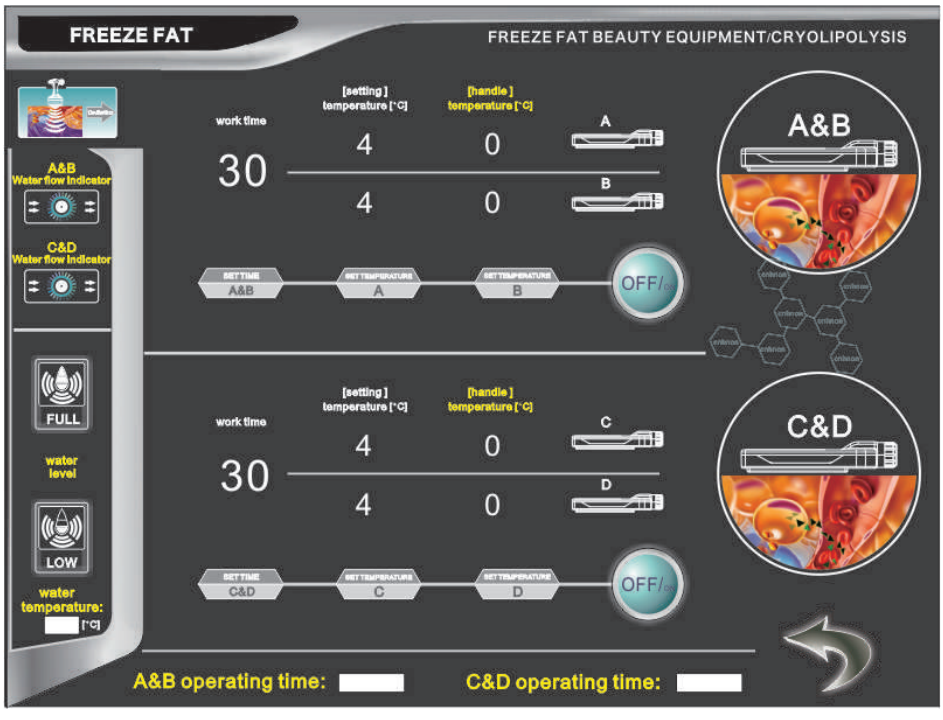

Press " work time " to adjust the time, Selection of Group A&B; by clicking " A " to set the Temperature you want, by clicking " B " to set the Temperature you want, Setting “4 or 5”, then Press " OFF/ " to start the cool pads A&B.

Temperature should be adjusted from high to low (usually 4~5℃ for 5 mins and then 0 ℃ for 10~15 mins)
Set the C&D group the same as the A&B.

TECHNICAL PARAMETERS
THE INSTALLATION PROCESS

Technical Parameters

Power	1000W
Voltage	200V–240V/Hz 110V–130V/Hz
Packing size	140*55*70CM
Vacuum pressure	–100kpa
Infrared light wavelength	650nm
RF Energy	50W
RF Frequency	1MHz
BIO Frequency	100Hz
Cavitation frequency	40KHZ
Mode	3 types

Treatment course and suggested Preferences

Handle	Technology	Parameters	Suggested Preferences	Suggested Treatment Course Setting
Cavitation (work with slimming gel&oil)	• Cavitation • Red Led	1–8	5–7	25~30min/treatment 10~12treatments/course 2–3 treatments/week
Cryolipolysis (work with anti–freeze membranes)	• Cooler • Infrared • Vacuum	–10℃~5℃ Or –5℃~5℃	5℃~3℃ → 0℃ → –3℃~ –5℃	3–5 treatment /course 20~25min/treatment 5℃ for 5min; 0℃for 5min; –3~–5℃for 10~15min; One treatments/Month
V10 (work with slimming oil)	• Cavitation • RF: • BIO • Infrared • Vacuum	1~10 1~10 1~15	Cavi: 6–7 RF: 3~5 BIO: 6~7	30~35min/treatment 10~12treatments/course One treatments/week
Cool pads (work with anti–freeze membranes)	• Cooler • vibrator	0 ℃	5℃~3℃ → 0℃	3–5 treatment /course 15~20min/treatment 5℃ for 5min; 0℃for 10~15min; One treatments/Month

The installation process

Host – On the left side of the shelf

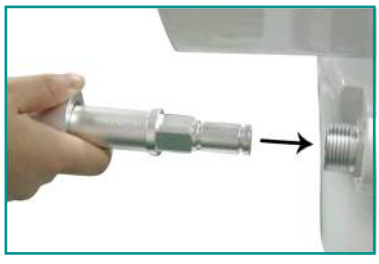

A

B

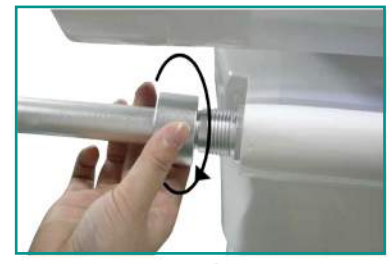

C

A

B

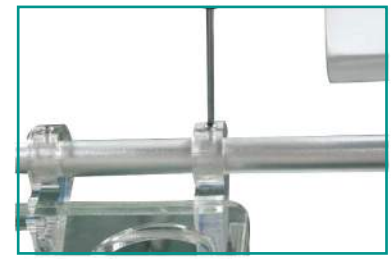

C

Host – On the right side of the shelf

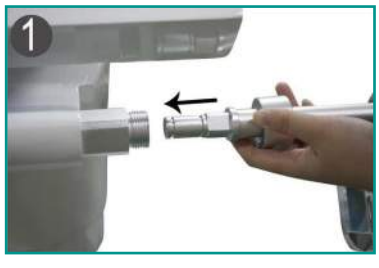

A

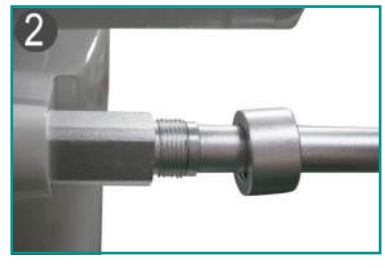

B

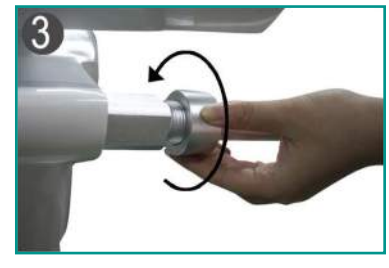

C

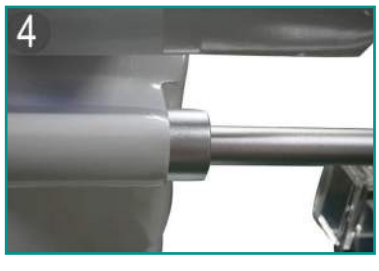

A

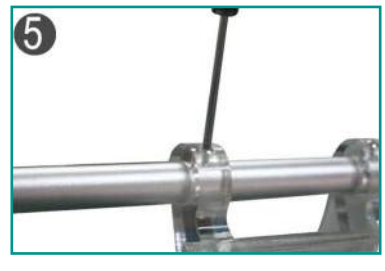

B

C

Handle

A

B

C

CHARMGIRL

Charmgirl beauty equipment ,the first brand of internation

Fashion • Innovation • Win-Win

Guangzhou Meizi Beauty Equipment Factory

Max: sales@meazi.com http:// www.charmgirl.cn

Add:West Of 5th Floor,Building F, Huixin Industrial Zone,Hetai Road,Hebian Village,Baiyun District,Guangzhou,Guangdong,China